


Pilot's Altimeter Calibration
Piper Navajo 11UT
Inst. Tag ALT1010J

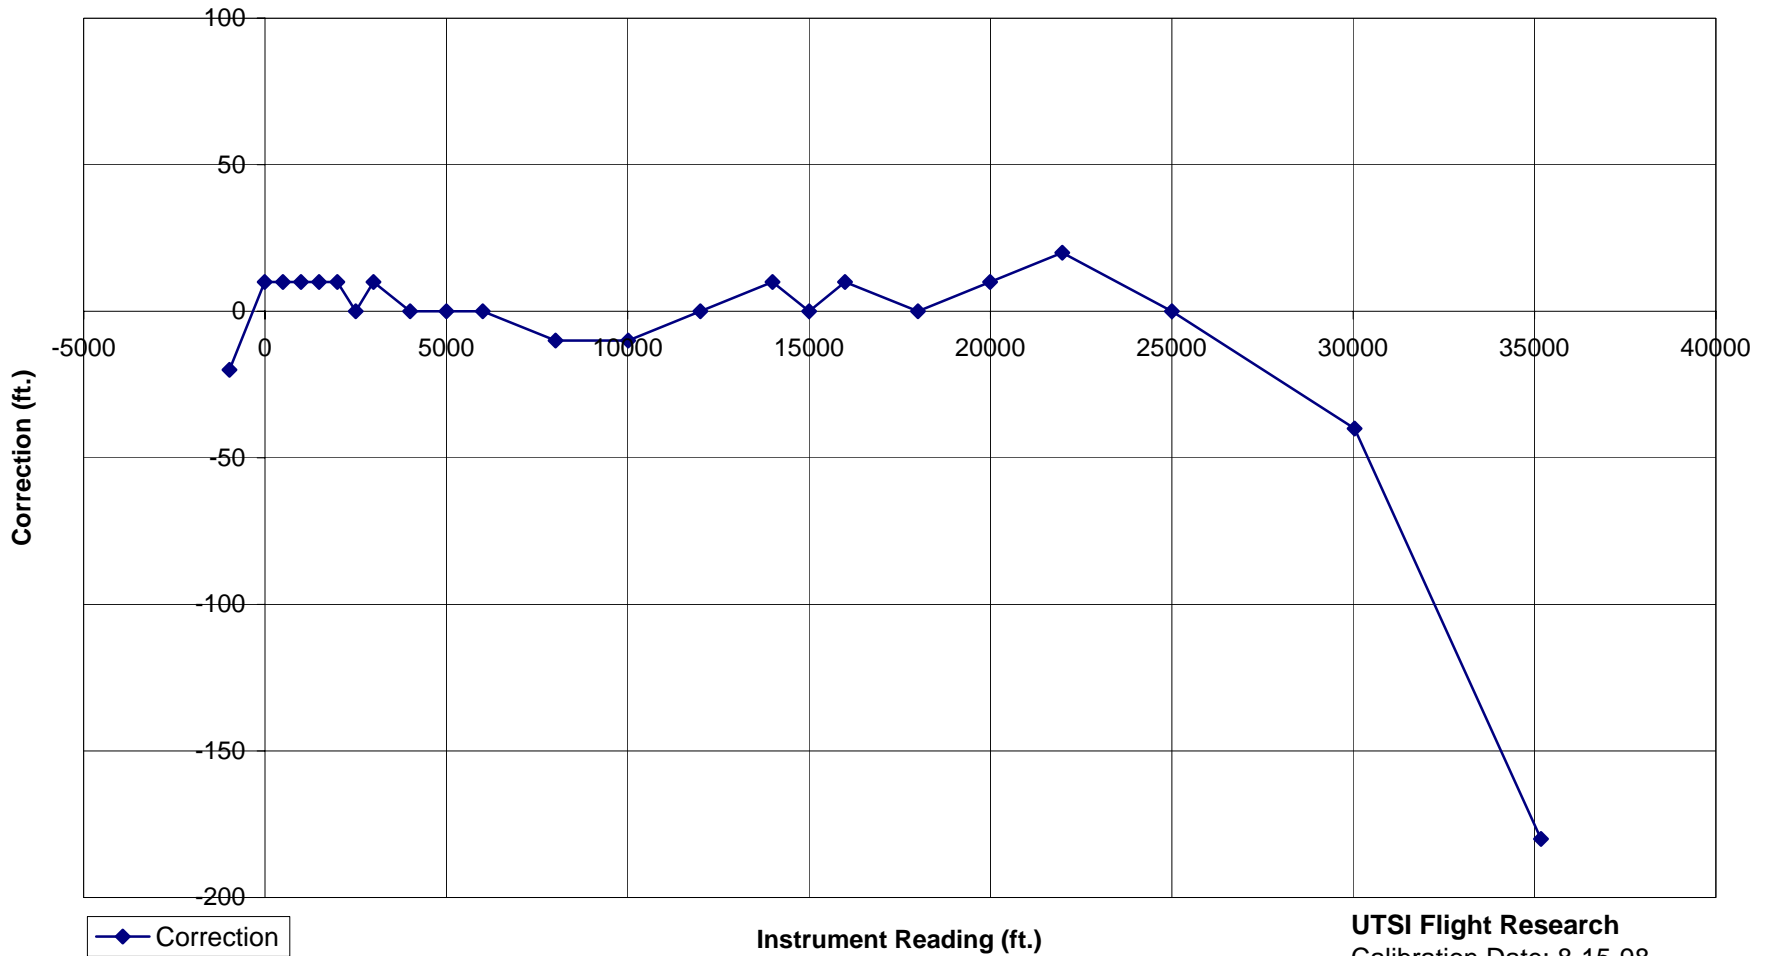

◆ Correction

Instrument Reading (ft.)

UTSI Flight Research
Calibration Date: 8-15-98
Inst. Serial #: AF56-7767
Calibrated by: P.T. & A. Inc.