


Elevator Position - All Student Consoles

Navajo N11UT

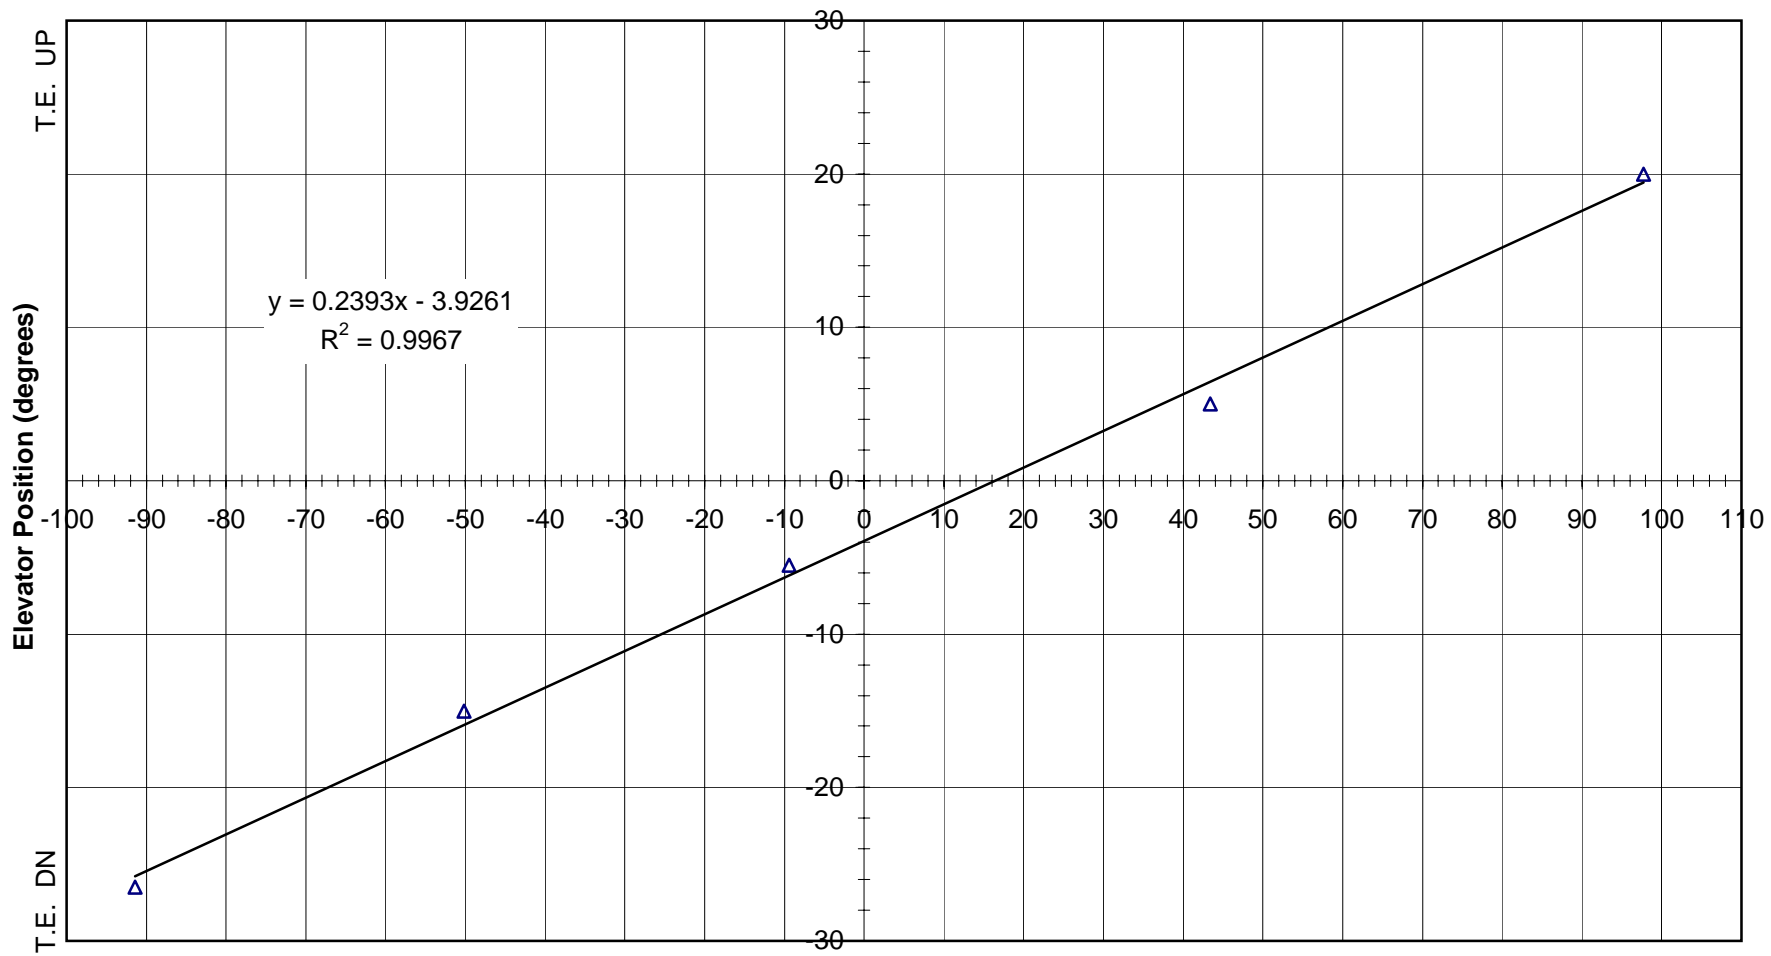

△ Calibration Points
— Linear Fit

Meter Reading

UTSI Flight Research
Calibration Date: 9/1/00
Inst. Serial # :N/A
Calibrated by: M. Leigh
Tag: POS1003J.XLS