


Instrument Calibration Chart

Airspeed - Center Console

Piper Saratoga N22UT

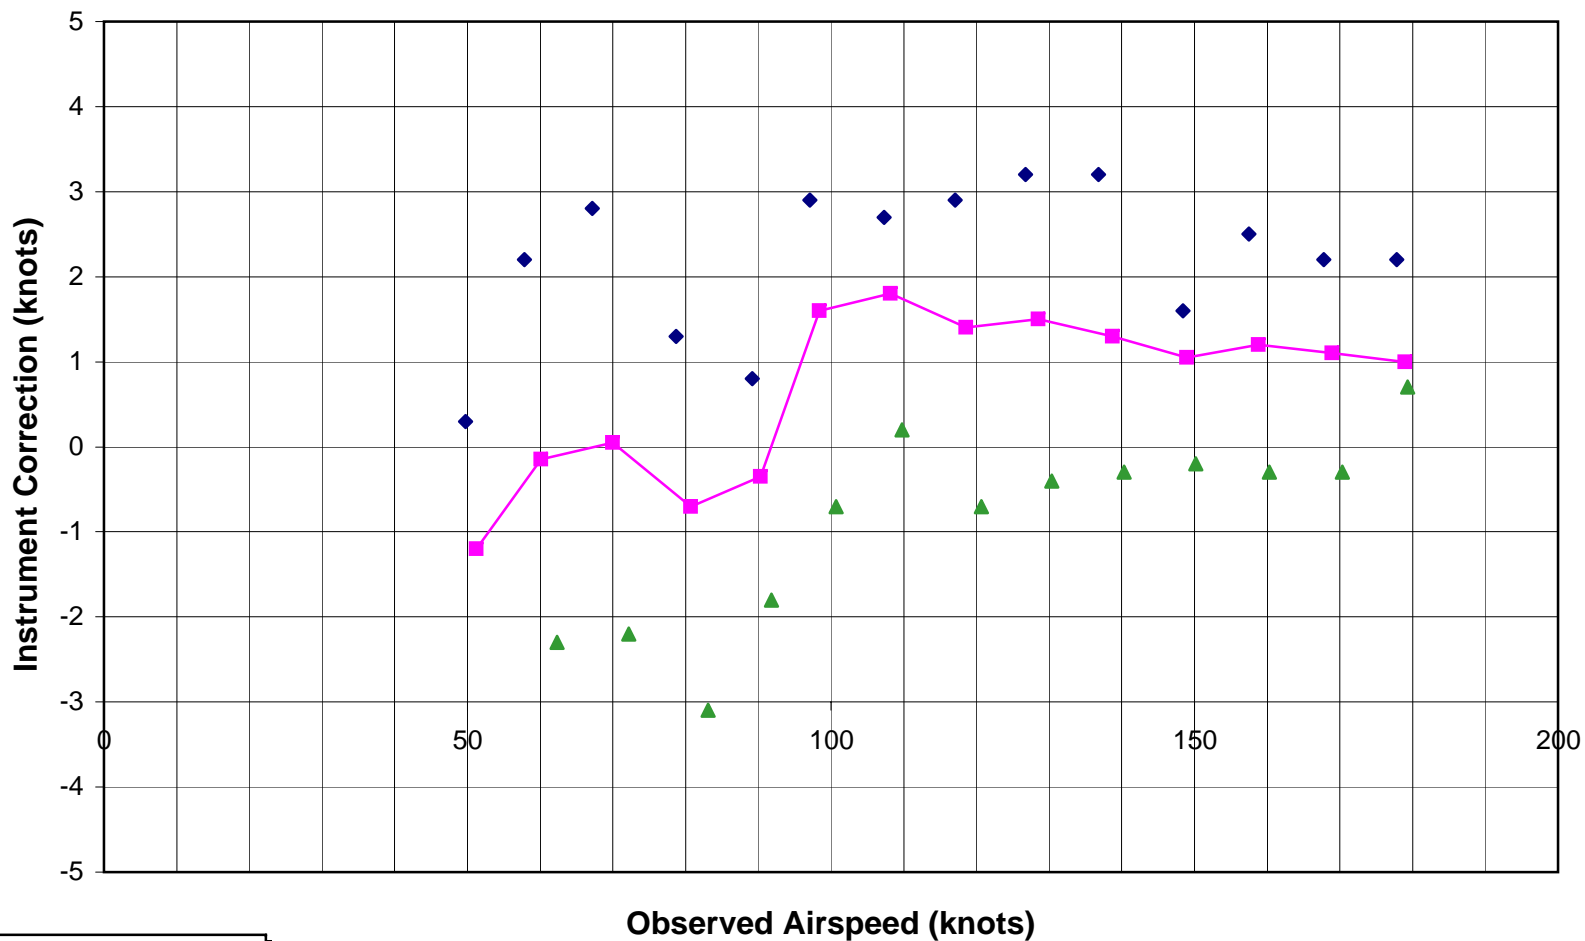

- ◆ Increasing
- ▲ Decreasing
- Tapped Value

UTSI Flight Research
Calibration Date: 8-14-00
Inst. Serial #: 15120
Calibrated by: M. Leigh
TAG: ASI1008S.XLS