


Instrument Calibration Chart

Manifold Pressure - Rear Console

Piper Saratoga N22UT

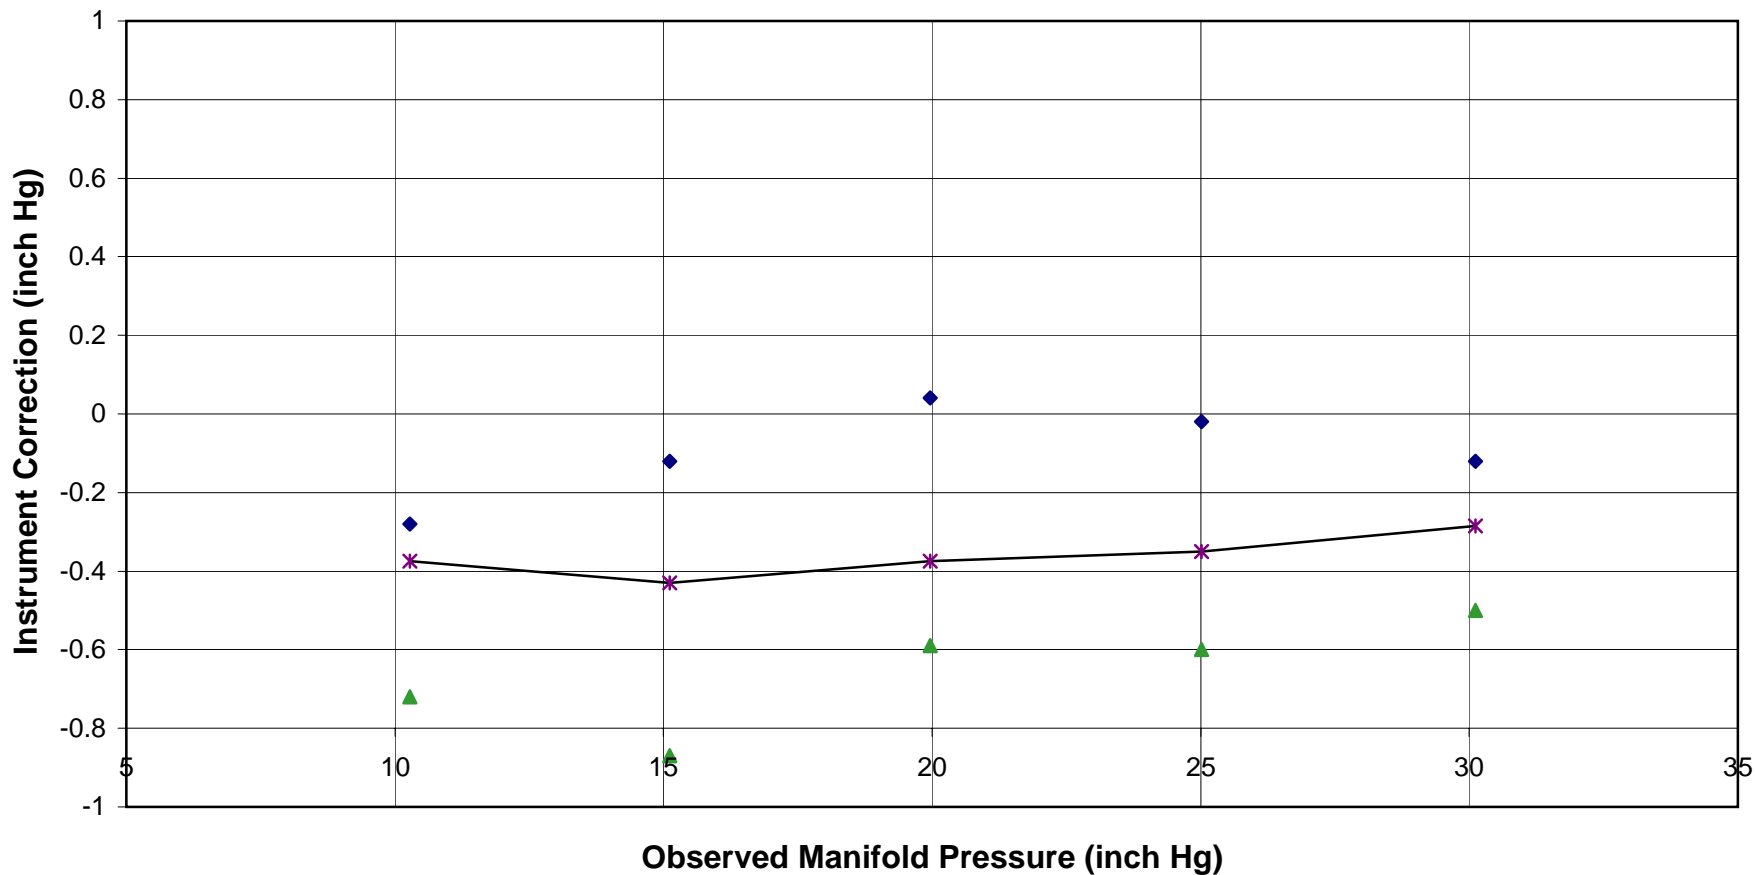

- ◆ Increasing
- ▲ Decreasing
- *— Tapped Value

UTSI Flight Research
Calibration Date: 8-16-00
ISN: I-05733
Calibrated by: M. Leigh
TAG: MAP1010S.XLS