


Normal Acceleration - All Student Consoles Saratoga N22UT

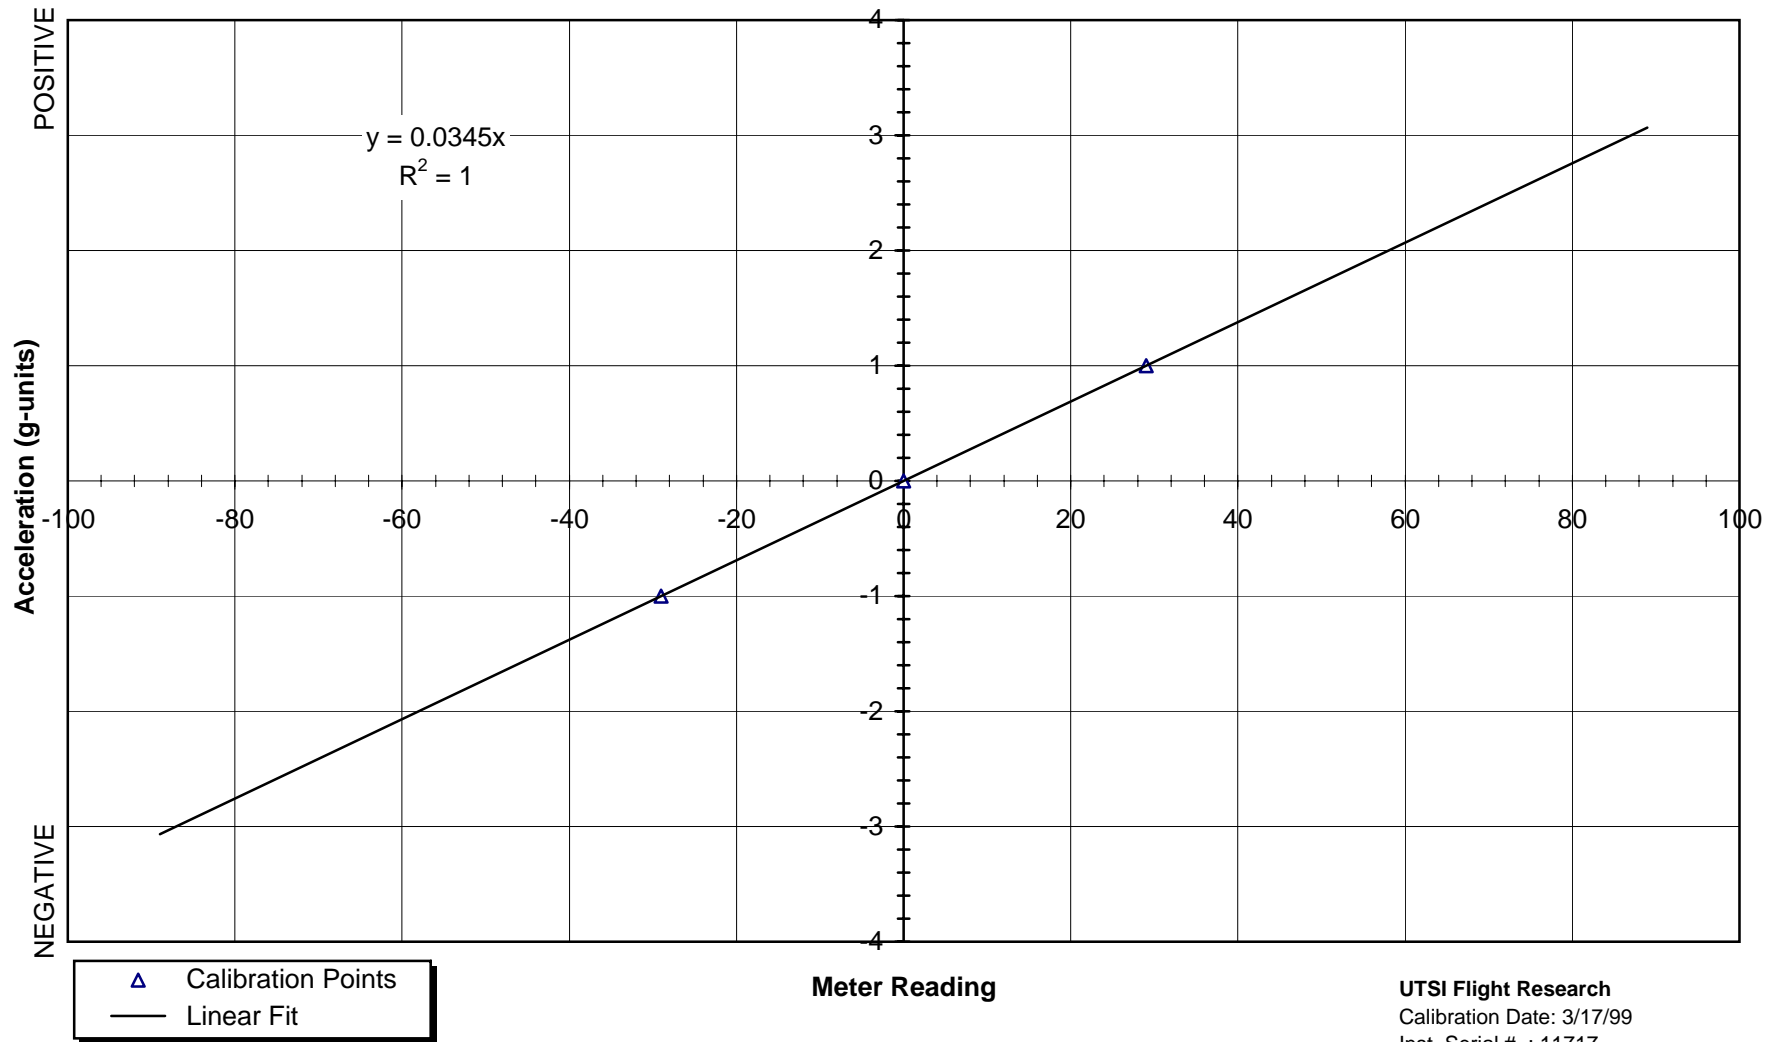

UTSI Flight Research
Calibration Date: 3/17/99
Inst. Serial # : 11717
Calibrated by: Leigh/Woodside
Tag: ACC1003S.XLS