


### Pitch Rate - All Student Consoles Saratoga N22UT

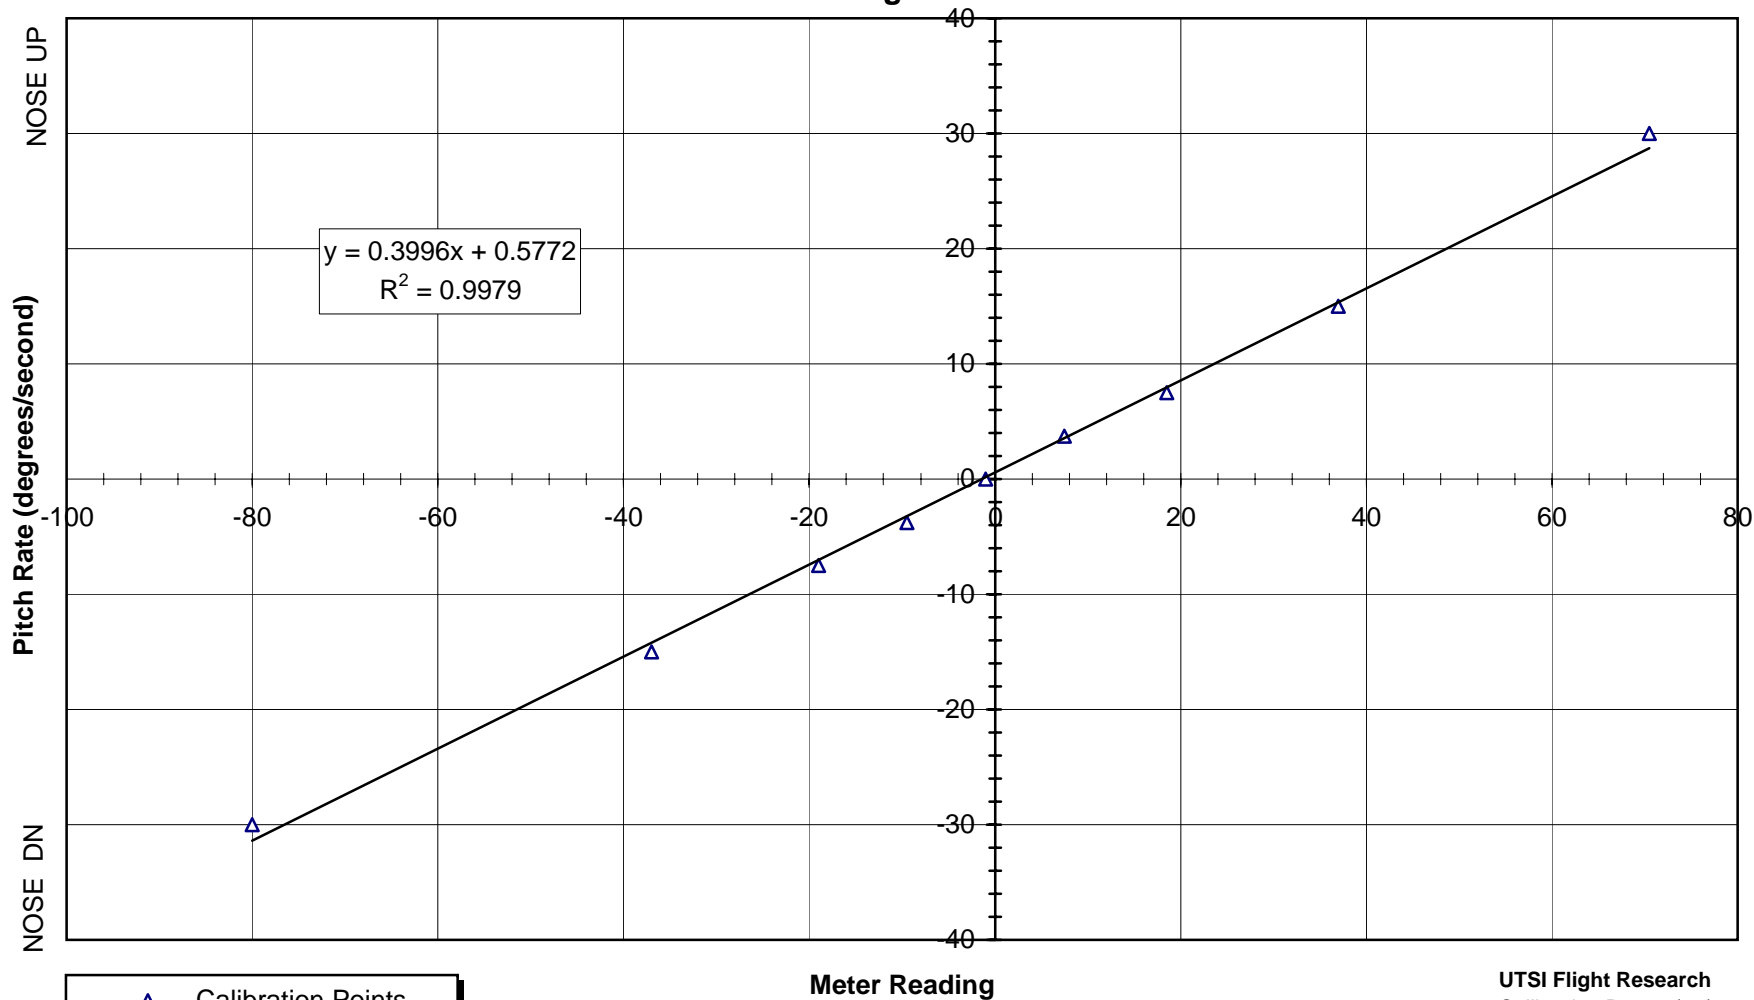

△ Calibration Points  
— Linear Fit

**UTSI Flight Research**  
Calibration Date: 6/18/98  
Inst. Serial # :N/A  
Calibrated by: M. Leigh  
Tag: GYR1008S.XLS